

**DYNAMIC
ABUTMENT**
SOLUTIONS

MULTI-UNIT
DAS SYSTEM

DYNAMIC
DAS SYSTEM

COMPATIBILITIES

COMPATIBILITIES AVAILABLE

ASTRA TECH OSSESOSPEED TX

Model: Aqua
Implant Ø: 3,5/4
Platform: Aqua (Estrecha) Code: 0004

Model: Lilac
Implant Ø: 4,5/5
Platform: Lilac (Ancha)
Code: 0005

BIOMET 3i OSSEOTITE CERTAIN

Model: Certain
Implant Ø: 3,25/4
Platform: 3,4
Code: 0001

Model: Certain
Implant Ø: 4/5
Platform: 4,1
Code: 0002

OSSTEM IMPLANT

Model: TS
Implant Ø: 3,5
Platform: Mini 3,5
Code: 0029

Model: TS
Implant Ø: 4/4,5/5/6/7
Platform: Regular
Code: 0030

MEGAGEN ANYRIDGE

Model: AnyRidge
Implant Ø: 3,5
Platform: Small
Code: 0015

Model: AnyRidge
Implant Ø: 4/4,5
Platform: Regular
Code: 0015

Model: AnyRidge
Implant Ø: 5/5,5
Platform: Wide
Code: 0015

NOBEL BIOCARE NOBEL ACTIVE

Model: Active
Implant Ø: 3,5
Platform: Narrow
Code: 0021

Model: Active
Implant Ø: 4,3/5
Platform: Regular
Code: 0022

Model: Active
Implant Ø: 5,5
Platform: Wide
Code: 0124

ZIMMER

Model: Screw-Vent
Implant Ø: 3,7/4,1
Platform: 3,5
Code: 0040

Model: Screw-Vent
Implant Ø: 4,7
Platform: 4,5
Code: 0041

Model: Screw-Vent
Implant Ø: 6
Platform: 5,7
Code: 0080

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 0.3 mm	α_s	α_c	GINGIVAL HEIGHT 1.2 mm	α_s	α_c	GINGIVAL HEIGHT 2 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c
R	31.322.001.01-2	43°	25°	31.322.001.02-2	25°	-	31.322.001.03-2	25°	-	31.322.001.04-2	20°	.	-	.	.
NR	31.312.001.01-2			31.312.001.02-2			31.312.001.03-2			31.312.001.04-2			-		

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG	SCANALOG
34.612.001.01-2	23.412.001.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.001.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.103.02-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	LAB SCANBODY
41.316.084.01-2	-	43.618.201.01-2	18	30.412.001.01-2
		43.624.201.01-2	24	
		43.632.201.01-2	32	

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.302.001.01-2	42.302.001.02-2	42.302.001.03-2	42.302.001.04-2

LIBRARY OPTIONS

- GH = Gingival Height α_s - Standard maximum angulation
- CH = Cement Height α_c - Captive maximum angulation
- IG = Adaptor 3mm α_d - Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 0.3 mm	α_s	α_c	GINGIVAL HEIGHT 1.2 mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c
R	31.323.002.01-2	45°	20°	31.323.002.02-2	25°	-	-	-	-	-	-	-	-	-	-
NR	31.313.002.01-2			31.313.002.02-2		-	-	-	-	-	-	-	-	-	-

DIGITAL ANALOG

SCANALOG

DIGITAL ANALOG

34.613.002.01-2	23.413.002.01-2
-----------------	-----------------

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.002.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.103.02-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	LAB SCANBODY
41.316.084.01-2	-	43.618.201.01-2	18	30.413.002.01-2
		43.624.201.01-2	24	
		43.632.201.01-2	32	

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.303.002.01-2	42.303.002.02-2	42.303.002.03-2	42.303.002.04-2

LIBRARY OPTIONS

- GH = Gingival Height
- CH = Cement Height
- IG = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_c = Direct to implant maximum angulation
- R = Rotational / Non-Engaging
- NR = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 1 mm	α_s	α_c	GINGIVAL HEIGHT 2 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c
R	31.323.004.01-2	45°	29°	31.323.004.02-2	30°	20°	31.323.004.03-2	25	-	31.323.004.04-2	20	-	-	-	-
NR	31.313.004.01-2			31.313.004.02-2			31.313.004.03-2			31.313.004.04-2			-		

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG	SCANALOG
34.613.004.01-2 34.613.004.02-2	23.413.004.02-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.004.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.105.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	LAB SCANBODY
41.316.076.01-2	-	43.618.201.01-2	18	30.413.002.01-2
		43.624.201.01-2	24	
		43.632.201.01-2	32	

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.303.004.01-2	42.303.004.02-2	42.303.004.03-2	42.303.004.04-2

LIBRARY OPTIONS

- GH** = Gingival Height α_s - Standard maximum angulation
- CH** = Cement Height α_c - Captive maximum angulation
- IG** = Adaptor 3mm α_c - Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 1 mm	α_s	α_c	GINGIVAL HEIGHT 2 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT mm	α_s	α_c
R	31.324.005.01-2	38°	23°	31.324.005.02-2	25°	15°	31.324.005.03-2	20	·	31.324.005.04-2	15	·	-	·	·
NR	31.314.005.01-2			31.314.005.02-2			31.314.005.03-2			31.314.005.04-2			-		

DIGITAL ANALOG

DIGITAL ANALOG

34.614.005.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.005.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.105.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.090.01-2	·	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.413.002.01-2

LIBRARY OPTIONS

- GH = Gingival Height
- CH = Cement Height
- IG = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_d = Direct to implant maximum angulation
- R = Rotational / Non-Engaging
- NR = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 1.7 mm	α_s	α_c	GINGIVAL HEIGHT 2.5 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT 5 mm	α_s	α_c
R	31.323.015.01-2	43°	23°	31.323.015.02-2	25°	15°	31.323.015.03-2	25°	-	31.323.015.04-2	20°	-	31.323.015.05-2	15°	-
NR	31.313.015.01-2			31.313.015.02-2			31.313.015.03-2			31.313.015.04-2			31.313.015.05-2		

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG

34.613.015.01-2	23.413.015.01-2
-----------------	-----------------

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.015.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.103.02-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.075.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.413.002.01-2

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.303.015.01-2	42.303.015.02-2	42.303.015.03-2	42.303.015.04-2

LIBRARY OPTIONS

- GH** = Gingival Height α_s - Standard maximum angulation
- CH** = Cement Height α_c - Captive maximum angulation
- IG** = Adaptor 3mm α_c - Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 1.5 mm	α_s	α_c	GINGIVAL HEIGHT 2 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT 5 mm	α_s	α_c
R	31.322.021.01-2	43°	24°	31.322.021.02-2	25°	20°	31.322.021.03-2	20°	25°	31.322.021.04-2	15°	25°	31.322.021.05-2	15°	20°
NR	31.312.021.01-2			31.312.021.02-2			31.312.021.03-2			31.312.021.04-2			31.312.021.05-2		

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG	SCANALOG
34.612.021.01-2	23.412.021.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.021.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.108.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.073.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.412.001.01-2

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.302.021.01-2	42.302.021.02-2	42.302.021.03-2	42.302.021.04-2

LIBRARY OPTIONS

- GH** = Gingival Height
- CH** = Cement Height
- IG** = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_d = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 1.3 mm	α_s	α_c	GINGIVAL HEIGHT 2 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT 5 mm	α_s	α_c
R	31.323.022.01-2	40°	19°	31.323.022.02-2	25°	14°	31.323.022.03-2	20°	30°	31.323.022.04-2	15	30	31.323.022.05-2	15°	20°
NR	31.313.022.01-2			31.313.022.02-2			31.313.022.03-2			31.313.022.04-2			31.313.022.05-2		

DIGITAL ANALOG **SCANALOG**

DIGITAL ANALOG	SCANALOG
34.613.022.01-2	23.413.022.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.022.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.108.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.075.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.413.002.01-2

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.303.022.01-2	42.303.022.02-2	42.303.022.03-2	42.303.022.04-2

LIBRARY OPTIONS

- GH** = Gingival Height α_s - Standard maximum angulation
- CH** = Cement Height α_c - Captive maximum angulation
- IG** = Adaptor 3mm α_c - Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
	1.2 mm														
R	-	30°	23°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.029.01-2			-			-			-			-		

DIGITAL ANALOG	SCANALOG
DIGITAL ANALOG	
34.613.029.01-2	23.412.029.01-2

SCANBODY OP				
SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.029.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.103.02-2

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.316.094.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY
30.412.001.01-2

LIBRARY OPTIONS

GH = Gingival Height α_s = Standard maximum angulation
CH = Cement Height α_c = Captive maximum angulation
IG = Adaptor 3mm α_o = Direct to implant maximum angulation

R = Rotational / Non-Engaging
NR = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
	1.1 mm														
R	-	42°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.030.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG	SCANALOG
34.613.030.01-2	23.413.030.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.030.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.103.02-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.079.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.413.002.01-2

LIBRARY OPTIONS

- GH** = Gingival Height α_s = Standard maximum angulation
- CH** = Cement Height α_c = Captive maximum angulation
- IG** = Adaptor 3mm α_c = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT 0.6 mm	α_s	α_c	GINGIVAL HEIGHT 1.5 mm	α_s	α_c	GINGIVAL HEIGHT 3 mm	α_s	α_c	GINGIVAL HEIGHT 4 mm	α_s	α_c	GINGIVAL HEIGHT 5 mm	α_s	α_c
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	31.322.040.03-2	20°	30°	31.322.040.04-2	15°	30°	31.322.040.05-2	10°	23°
NR	31.312.040.01-2			31.312.040.02-2			31.312.040.03-2			31.312.040.04-2			31.312.040.05-2		
NR (Friction-Fit)	31.312.042.01-2			-			-			-			-		

DIGITAL ANALOG SCANALOG

DIGITAL ANALOG	SCANALOG
34.612.040.01-2	23.412.040.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.040.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.105.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.412.001.01-2

MULTI-UNIT

	GINGIVAL HEIGHT 1 mm	GINGIVAL HEIGHT 2 mm	GINGIVAL HEIGHT 3 mm	GINGIVAL HEIGHT 4 mm
R	42.302.040.01-2	42.302.040.02-2	42.302.040.03-2	42.302.040.04-2

LIBRARY OPTIONS

- GH** = Gingival Height α_s = Standard maximum angulation
- CH** = Cement Height α_c = Captive maximum angulation
- IG** = Adaptor 3mm α_d = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
	0,4 mm			1,5 mm			mm			mm			mm		
R	31.323.041.01-2	45°	30°	31.323.041.02-2	30°	25°	-	.	.	-	.	.	-	.	.
NR	31.313.041.01-2			31.313.041.02-2			-			-			-		
NR (Friction-Fit)	31.313.043.01-2			-			-			-					

DIGITAL ANALOG

SCANALOG

DIGITAL ANALOG	SCANALOG
34.613.041.01-2	23.413.041.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.041.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.105.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.413.002.01-2

LIBRARY OPTIONS

- GH** = Gingival Height
- CH** = Cement Height
- IG** = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_{ic} = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
	0.4 mm			mm			mm			mm			mm		
R	31.324.080.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.080.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DIGITAL ANALOG

DIGITAL ANALOG
34.614.080.01-2

SCANBODY OP

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.080.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.601.104.01-2

DYNAMIC SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.071.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.414.003.01-2

LIBRARY OPTIONS

- GH** = Gingival Height
- CH** = Cement Height
- IG** = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_o = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging

STANDARD DYNAMIC TIBASE

	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c	GINGIVAL HEIGHT	α_s	α_c
	1.4 mm			mm			mm			mm			mm		
R	31.324.124.01-2	42°	19°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.124.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DIGITAL ANALOG

SCANBODY OP

DIGITAL ANALOG
34.614.124.01-2

SCANBODY	PEEK PINS TYPE A	PEEK PINS TYPE B	PEEK PINS TYPE C	mm
54.315.124.21-2	49.414.000.01-2	49.414.000.02-2	49.414.000.03-2	6
	49.415.000.01-2	49.415.000.02-2	49.415.000.03-2	9
	49.416.000.01-2	49.416.000.02-2	49.416.000.03-2	13

SCREWDRIVER 43.625.108.01-2

DYNAMIC SCREWS


DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.320.075.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

LAB SCANBODY

30.414.003.01-2


LIBRARY OPTIONS

- GH** = Gingival Height
- CH** = Cement Height
- IG** = Adaptor 3mm
- α_s = Standard maximum angulation
- α_c = Captive maximum angulation
- α_{ic} = Direct to implant maximum angulation
- R** = Rotational / Non-Engaging
- NR** = Non Rotational / Engaging




This printed version is probably
outdated and may not include
all products or compatibilities.
Scan and download the latest
version of this catalogue.
www.dynamicabutment.us

DAS LIBRARIES

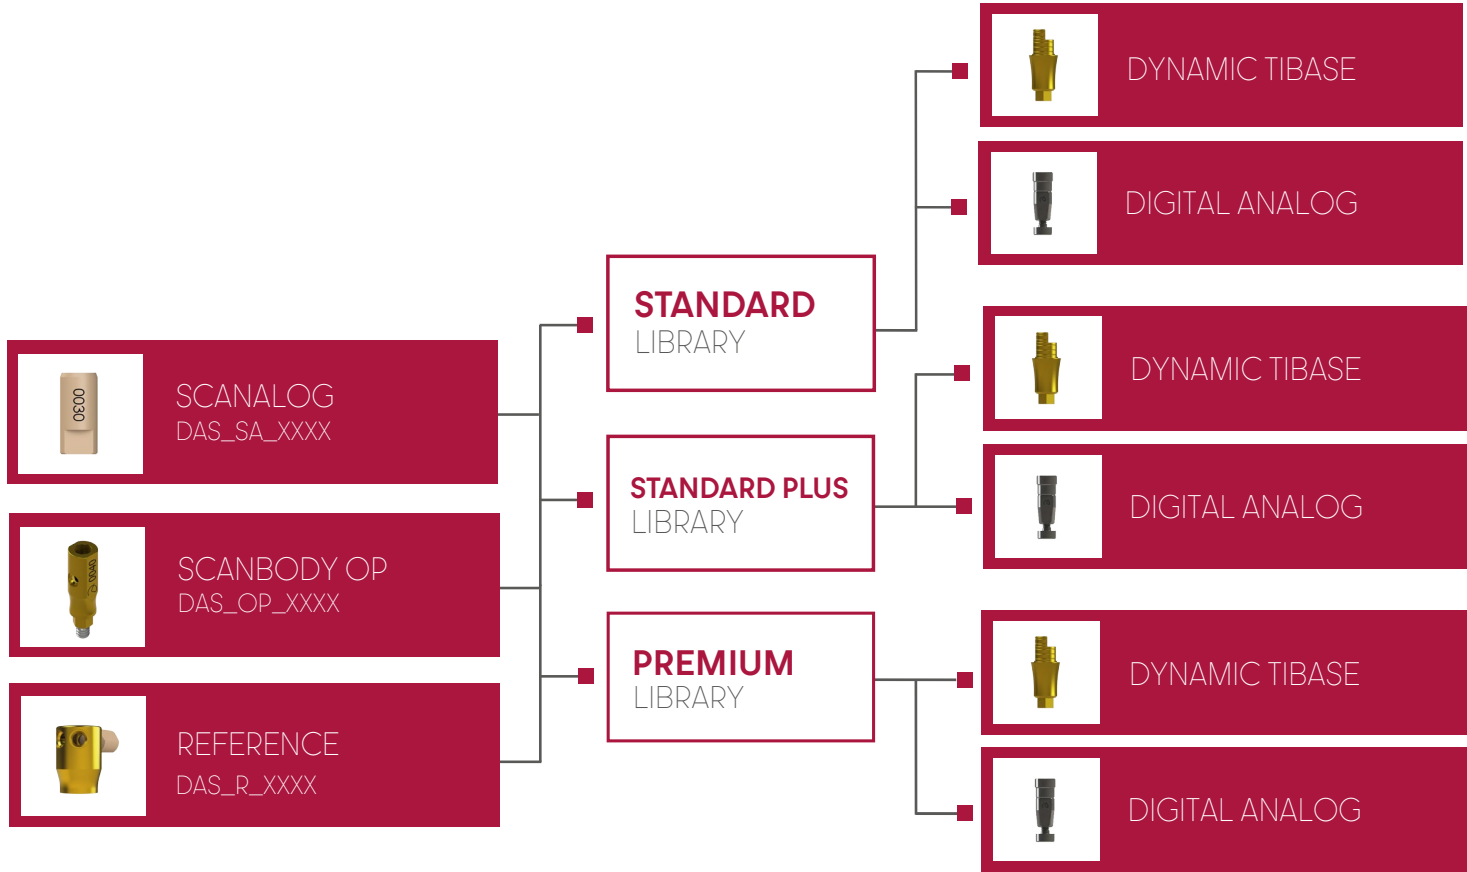


MULTI-UNIT DAS LIBRARIES

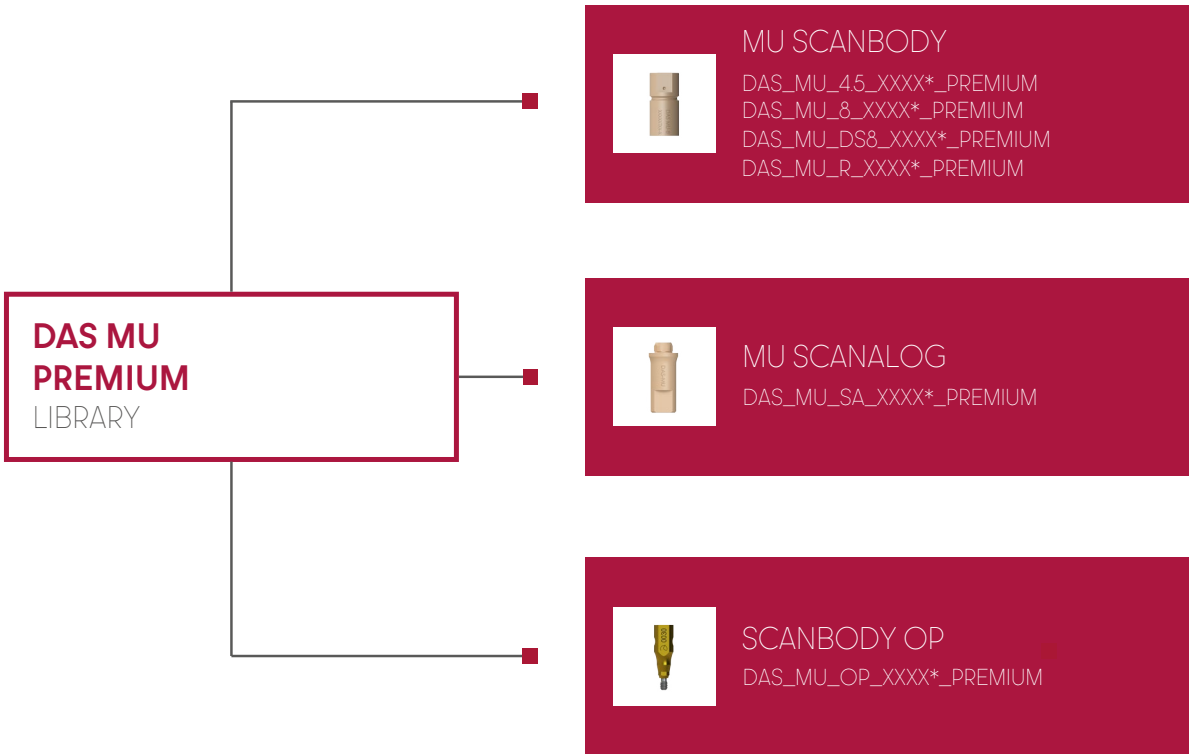

DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.316.073.01-2	1.6	20 Ncm	7.3	2.2	4.87	5.56	1.74	2.3	conical	35°	45° Chamfer	HEXALOBULAR 1.70
41.316.076.01-2	1.6	20 Ncm	7.6	3.6	6.1	-	1.5	2.3	straight	-	Semi-sphere	
41.316.084.01-2	1.6	20 Ncm	8.4	3.5	6.8	-	1.6	2.3	straight	-	Semi-sphere	
41.316.094.01-2	1.6	20 Ncm	9.4	2.9	7.65	8	1.4	2.3	conical	45°	45° Chamfer	
41.317.071.01-2	N1-72	25 Ncm	7.1	2.5	5.56	5.65	1.45	2.3	conical	70°	45° Chamfer	
41.318.075.01-2	1.8	25 Ncm	7.5	3.3	6.1	-	1.4	2.3	straight	-	Semi-sphere	
41.320.075.01-2	2	25 Ncm	7.5	2.75	5.93	6.18	1.32	2.3	conical	35°	45° Chamfer	
41.320.079.01-2	2	25 Ncm	7.9	3.3	6.33	6.5	1.4	2.3	conical	45°	45° Chamfer	
41.320.090.01-2	2	25 Ncm	9	4	7.5	-	1.5	2.3	straight	-	Semi-sphere	

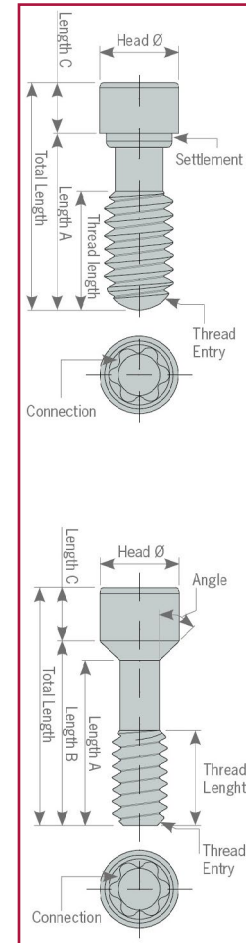

SCREWDRIVER ADAPTOR

Ref. 43.621.415.01-2

Tiny Screwdriver with manual handle
Length: 21 mm



DYNAMIC SCREWDRIVERS

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment System.
Lengths: 18, 24, 32 mm

Hexalobular 1,70 mm. Length: 18 mm
Ref. 43.618.201.01-2



Hexalobular 1,70 mm. Length: 24 mm
Ref. 43.624.201.01-2



Hexalobular 1,70 mm Length: 32 mm
Ref. 43.632.201.01-2



COMPLEMENTS

Manual handle

Made of stainless steel.
They are used to connect screwdriver bits with the contra-angle connection



Large manual handle for laboratory

Ref. 49.601.000.03-2

Ideal to manipulate models in the laboratory
Length: 55.65 mm



Manual handle for clinic

Ref. 49.601.000.01-2

Clinic handle: used to position the prosthesis in the mouth prior to torque control in the clinic.
Length: 15.65 mm



Dynamic Screw Transfer

Ref. 49.413.000.01-2

Manual torque wrench adapter prosthetic

Piece to connect the screwdriver with contra-angle connection to the torque wrench.



Universal Manual torque wrench adapter
Ref. 49.604.000.05-2
4 mm Square connection



Straumann Manual torque wrench adapter
Ref. 49.604.000.07-2
Straumann connection




Nobel Biocare Manual torque wrench adapter
Ref. 49.604.000.08-2



MIS Manual torque wrench adapter
Ref. 49.604.000.09-2

DYNAMIC MILLING TOOL SPECIFICATIONS

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		$\varnothing c$	α	Lc	Lu	$\varnothing v$	$\varnothing s$	Lt
BEGO RS/RSX 3° ASTRA EVOLUTION 3.0° *Only for titanium and soft materials	33.325.472.01-2	1.4	25	0.4	4.7	0.5	3	50
	33.425.472.01-2	1.4	25	0.4	4.7	0.5	4	50
	33.625.472.01-2	1.4	25	0.4	4.7	0.5	6	50
STRAUMANN BONE LEVEL NP STRAUMANN BONE LEVEL RP MEDENTIS ICX TEMPLANT 4:1 STRAUMANN SYNOCCTA 3.5 MEDENTIS ICX NARROW	33.315.804.01-2	1.6	15	0.7	8	0.65	3	50
	33.415.804.01-2	1.6	15	0.7	8	0.65	4	50
	33.615.804.01-2	1.6	15	0.7	8	0.65	6	50
ANTHOGRYR AXIOM RG/PX XNP ANTHOGRYR AXIOM RG/PX RP ANTHOGRYR AXIOM RG/PX WP	33.320.704.01-2	1.6	20	0.7	7	0.8	3	50
	33.420.704.01-2	1.6	20	0.7	7	0.8	4	50
	33.620.704.01-2	1.6	20	0.7	7	0.8	6	50
ASTRA EVOLUTION 3.6 ANKYLOS ALPHABIO CONICAL STANDARD CON- NECTION LASAK BIONIQ QR NICODENT GM ANKYLOS BALANCE BASE	33.330.734.01-2	1.6	30	0.7	7.3	0.8	3	50
	33.430.734.01-2	1.6	30	0.7	7.3	0.8	4	50
	33.630.734.01-2	1.6	30	0.7	7.3	0.8	6	50
NOBEL BIOCARE ACTIVE NP NOBEL BIOCARE ACTIVE 3.0 LASAK BIONIQ QN	33.335.754.01-2	1.6	35	0.7	7.5	0.65	3	50
	33.435.754.01-2	1.6	35	0.7	7.5	0.65	4	50
	33.635.754.01-2	1.6	35	0.7	7.5	0.65	6	50
OSSTEM TS NP CAMLOG SCREW LINE 3.8 NP CAMLOG SCREW LINE 4.3 RP KLOCKNER VEGA NV XIVE S 3.4 BIOTECH DENTAL KONTACT XNP BIOTECH DENTAL KONTACT RP DIO UF NP CAMLOG SCREW-LINE 3.3	33.345.804.01-2	1.6	45	0.7	8	0.65	3	50
	33.445.804.01-2	1.6	45	0.7	8	0.65	4	50
	33.645.804.01-2	1.6	45	0.7	8	0.65	6	50
MIS C1 NP MIS M4 NP CONEOLOG 3.8 CONEOLOG 4.3 ASTRA YELLOW ALPHABIO CONICAL HEX CONNECTION	33.360.754.01-2	1.6	60	0.7	7.5	0.65	3	50
	33.460.754.01-2	1.6	60	0.7	7.5	0.65	4	50
	33.660.754.01-2	1.6	60	0.7	7.5	0.65	6	50
BIOMET 3i CERTAIN NP ASTRA AQUA	33.390.754.01-2	1.6	90	0.7	7.5	0.65	3	50
	33.490.754.01-2	1.6	90	0.7	7.5	0.65	4	50
	33.690.754.01-2	1.6	90	0.7	7.5	0.65	6	50
ASTRA EVOLUTION 4.2	33.350.775.01-2	1.7	50	0.7	7.7	0.8	3	50
	33.450.775.01-2	1.7	50	0.7	7.7	0.8	4	50
	33.650.775.01-2	1.7	50	0.7	7.7	0.8	6	50
BIOMET 3i CERTAIN RP NOBEL BIOCARE BRANEMARK NP NOBEL BIOCARE REPLACE NP MEGAGEN ANYRIDGE RP BIOMET 3i CERTAIN WP	33.390.805.01-2	1.7	90	0.7	8	0.65	3	50
	33.490.805.01-2	1.7	90	0.7	8	0.65	4	50
	33.690.805.01-2	1.7	90	0.7	8	0.65	6	50

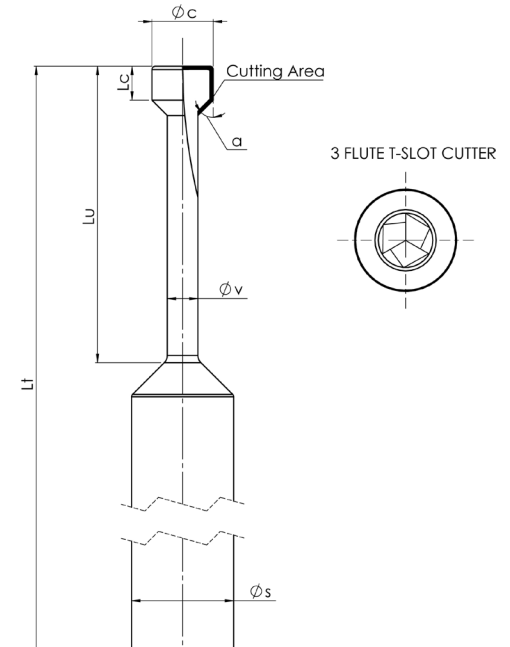

DYNAMIC MILLING TOOL SPECIFICATIONS

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		Øc	α	Lc	Lu	Øv	Øs	Lt
BEGO S/RI 3.25-3.75 BEGO S/RI 4.1 BEGO S/RI 4.5 BEGO S/RI 5.50 STRAUMANN SCREW-RETAINED NC/RC BEGO MULTI-PLUS	33.335.676.01-2	1.8	35	1	6,7	0,9	3	50
	33.435.676.01-2	1.8	35	1	6,7	0,9	4	50
	33.635.676.01-2	1.8	35	1	6,7	0,9	6	50
KLOCKNER ESSENTIAL CONE 4.5 DIRECTO IMPLANTE KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 12° KLOCKNER ESSENTIAL CONE 4.5 OCTA- CONE 25° KLOCKNER VEGA RV XIVE S 3.8 XIVE S 4.5 BIOHORIZONS 3.0 STRAUMANN SYNOCCTA 6.5 STRAUMANN BLX RB STRAUMANN BLX WB STRAUMANN TLX NT STRAUMANN TLX RT STRAUMANN TLX WT	33.345.856.01-2	1.8	45	1	8,5	0,9	3	50
	33.445.856.01-2	1.8	45	1	8,5	0,9	4	50
	33.645.856.01-2	1.8	45	1	8,5	0,9	6	50
MIS C1 RP PALTOP UNIVERSAL MULTI UNIT MIS C1 WP S&M PREMIUM KHONO 3.3 S&M PREMIUM KHONO 3.8 S&M OUTLINK 3.3 S&M OUTLINK 4.1 S&M PREMIUM KHONO 4.25 BREDENT SKY NP BREDENT SKY RP ADIN TOUAREG/CLOSEFIT NP ADIN TOUAREG/CLOSEFIT UNP CAMLOG CONELO 3.3 GLOBAL D (TEKKA) EASY IMPLANT MINI	33.360.756.01-2	1.8	60	1	7,5	0,9	3	50
	33.460.756.01-2	1.8	60	1	7,5	0,9	4	50
	33.660.756.01-2	1.8	60	1	7,5	0,9	6	50
ZIMMER SCREW-VENT 3.5 ZIMMER SCREW-VENT 4.5 ASTRAEVOLUTION UNIT ABUTMENT ZIMMER TYPE 5.7	33.370.716.01-2	1.8	70	1	7,1	0,9	3	50
	33.470.716.01-2	1.8	70	1	7,1	0,9	4	50
	33.670.716.01-2	1.8	70	1	7,1	0,9	6	50
NOBEL BIOCARE BRANEMARK RP NOBEL BIOCARE MULTI-UNIT RP BIOMET 3i OSSEOTITE NP BTI EXTERNAL CONNECTION NP BTI INTERNAL CONNECTION NP MIS MULTI-UNIT ST KEYSTONE PRIMA NP KEYSTONE PRIMA RP KEYSTONE PRIMA WP NEOSS PROACTIVE 3.4 NEOSS PROACTIVE 4.1 BIOMET 3i OSSEOTITE WP BTI EXTERNAL CONNECTION WP BTI MULTI-IM UNIVERSAL RP ANTHOGYRD MULTI-UNIT 4.8 BEGO MINI BTI INTERNAL WP LASAK MULTI-UNIT ON/OR SIC SICACE 3.3 SIC SICACE 4.2	33.390.716.01-2	1.8	90	1	7,1	0,9	3	50
	33.490.716.01-2	1.8	90	1	7,1	0,9	4	50
	33.690.716.01-2	1.8	90	1	7,1	0,9	6	50

DYNAMIC MILLING TOOL SPECIFICATIONS

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		\varnothing_c	α	L_c	L_u	\varnothing_v	\varnothing_s	L_t
STRAUMANN INTERNAL OCTAGON RP STRAUMANN INTERNAL OCTAGON 6,5	33.315.708.01-2	2	15	1	7	1	3	50
	33.415.708.01-2	2	15	1	7	1	4	50
	33.615.708.01-2	2	15	1	7	1	6	50
STRAUMANN SYNOCTA RP	33.330.708.01-2	2	30	1	7	1	3	50
	33.430.708.01-2	2	30	1	7	1	4	50
	33.630.708.01-2	2	30	1	7	1	6	50
NOBEL BIOCARE ACTIVE RP NOBEL BIOCARE ACTIVE WP	33.335.758.01-2	2	35	1	7,5	1	3	50
	33.435.758.01-2	2	35	1	7,5	1	4	50
	33.635.758.01-2	2	35	1	7,5	1	6	50
OSSTEM TS RP CAMLOG SCREW-LINE 5.0 CAMLOG SCREW-LINE 6.0	33.345.808.01-2	2	45	1	8	1	3	50
	33.445.808.01-2	2	45	1	8	1	4	50
	33.645.808.01-2	2	45	1	8	1	6	50
NOBEL BIOCARE REPLACE RP ASTRA LILAC NOBEL BIOCARE REPLACE WP ASTRA EVOLUTION 4.8 NOBEL BIOCARE BRANEMARK WP ASTRA EVOLUTION 5.4 NOBEL BIOCARE REPLACE 6.0	33.390.958.01-2	2	90	1	9,5	1	3	50
	33.490.958.01-2	2	90	1	9,5	1	4	50
	33.690.958.01-2	2	90	1	9,5	1	6	50



TALLADIUM GUARANTEE

TERMS AND CONDITIONS

These guarantee terms and conditions ("T&C") cover the entire range of Talladium products ("Products"), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician ("Clinician") and of the dental technician ("Technician") and not for the benefit of third parties or institutions, including patients.

GUARANTEE PERIOD

TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

GUARANTEE SCOPE

Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

QUALITY: If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

SAFETY: If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment or Dynamic Titanium Base system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

CLAIM REQUIREMENTS AND PROCEDURE

To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:

- a) The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
- b) This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
- c) A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
- d) Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
- e) All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
- f) The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C. Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

GENERAL LIMITATIONS OF THIS GUARANTEE

With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes. In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.


GUARANTEE EXCLUSIONS

TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Clinical screws that have been in the mouth for more than 2 years.
- Those products that are not used with the accessories and parts marketed by Talladium España

AMENDMENT OR SUSPENSION OF THE GUARANTEE

TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.



This printed version is probably
outdated and may not include
all products or compatibilities.
Scan and download the latest
version of this catalogue.

www.dynamicaabutment.us